

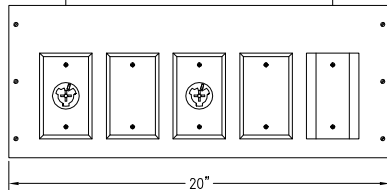


TOP VIEW

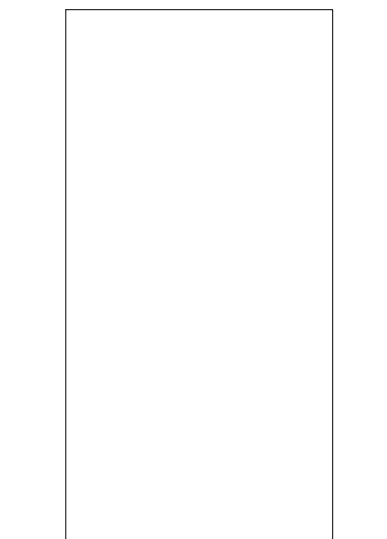

RIGHT SIDE VIEW

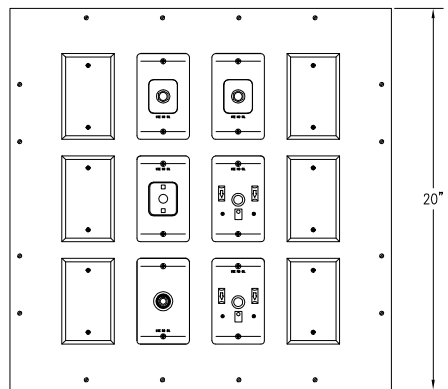


FRONT VIEW

**PLEASE SPECIFY:**


CEILING HEIGHT: \_\_\_\_\_

COLUMN HEIGHT: \_\_\_\_\_

QTY. OF COLUMNS: \_\_\_\_\_

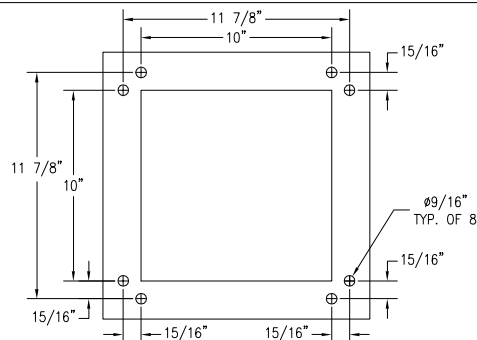

MOUNTING DETAIL

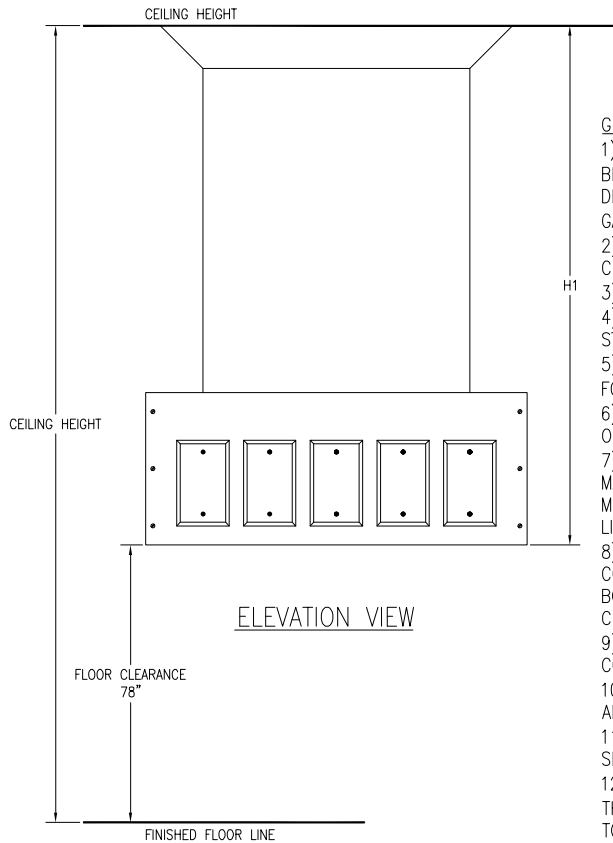

ELEVATION VIEW

COLUMN HEIGHT  
(15" TO 42" IN 3" INCREMENTS)

- H1=COLUMN HEIGHT
- =15"
- =18"
- =21"
- =24"
- =27"
- =30"
- =33"
- =36"
- =39"
- =42"

**GENERAL NOTES:**

- 1). THE POST GLOVER LIFELINK CEILING COLUMN SHALL BE A 14" x 14" SQUARE CHASE WITH A 20" x 20" x 8" DEVICE CHASSIS. COLUMN TO BE CONSTRUCTED OF 16 GAGE STAINLESS STEEL WITH A #4 SATIN FINISH.
- 2). CEILING HEIGHT IS TO BE DETERMINED BY THE CUSTOMER.
- 3). MOUNTING STRUCTURE SUPPLIED BY OTHERS.
- 4). CONTRACTOR HAS FINAL RESPONSIBILITY FOR THE STRENGTH AND STABILITY OF THE MOUNTING STRUCTURE.
- 5). A STAINLESS STEEL CEILING COLLAR (MADE FROM FOUR SECTIONS) IS SUPPLIED WITH THE UNIT.
- 6). UP TO 12 GAS SERVICE OUTLETS CAN BE MOUNTED ON THE FACE OF THE CEILING COLUMN.
- 7). MEDICAL GAS OUTLETS MAY BE PROVISIONS ONLY OR MAY BE PROVIDED BY MANUFACTURER OF PEDESTAL. MEDICAL GAS OUTLETS ARE TO BE CONNECTED TO GAS LINES BY DIVISION 15 TRADE.
- 8). ANY COMBINATION OF ELECTRICAL, GROUND JACKS, COMPUTER OUTLETS, COMMUNICATION DEVICES, AND BOTTLE SLIDES CAN BE MOUNTED ON THE FOUR DEVICE CHASSIS SIDES.
- 9). WIRE IN ACCORDANCE WITH NATIONAL ELECTRICAL CODE USING COPPER TYPE WIRE.
- 10). ALL DEVICES ARE FACTORY INSTALLED ON THE SIDE AND ON THE BOTTOM OF THE COLUMN.
- 11). ALL SIDES OF CEILING COLUMN CHASE PROVIDES SERVICE ACCESS.
- 12). ELECTRICAL AND GAS TUBING SHALL ENTER THROUGH A 10" x 10" ACCESS OPENING LOCATED AT TOP OF PANEL.

FOR:	S.O. NUM.:
------	------------

STD. B.O.M.: ORPD05001.xls ACAD STD.: ORDP05001.dwg



**POST GLOVER LIFELINK**  
4750 OLYMPIC BLVD. BLDG. B  
ERLANGER, KY U.S.A. 41018 (859) 283-5900  
COPYRIGHT © 2005

THIS DOCUMENT AND THE INFORMATION IT CONTAINS ARE THE PROPERTY OF POST GLOVER LIFELINK. IT IS DISCLOSED FOR THE PURPOSE FOR WHICH IT IS FURNISHED AND SHALL NOT BE DUPLICATED OR DISTRIBUTED.

TITLE/DESCRIPTION: OPERATING ROOM PEDESTAL TYPE: CEILING COLUMN, GENERAL LAYOUT AND ELEVATION VIEW PAGE 1 OF 2			
DFTR: JJM	DATE: 03/10/05	DWG. NO.: <b>ORDP05001</b>	REV.: 00