


GENERAL NOTES:

- 1). ENCLOSURE IS A ONE-PIECE ASSEMBLY AND IS FABRICATED OF 12 GAGE POLISHED STAINLESS STEEL IN ACCORDANCE WITH UL STANDARD 50.
- 2). ELECTRICAL AND GAS TUBING SHALL ENTER THROUGH A 8" x 8" ACCESS OPENING LOCATED AT BOTTOM OF PANEL.
- 3). ELECTRICAL RECEPTACLES AND GROUND JACK RECEPTACLES CAN BE MAXIMUM OF FOUR RECEPTACLES WIDE.
- 4). MEDICAL GAS OUTLETS MAY BE PROVISIONS ONLY OR MAY BE PROVIDED BY MANUFACTURER OF PEDESTAL. MEDICAL GAS OUTLETS ARE TO BE CONNECTED TO GAS LINES BY DIVISION 15 TRADE.
- 5). MEDICAL GAS OUTLETS TO BE CONSOLE STYLE. MAX. OF THREE GAS OUTLETS WIDE. PLEASE STAGGER MULTIPLE ROWS OF GAS OUTLETS FOR TUBING CLEARANCE.
- 6). 10"L x 10"W x 6"H MOUNTING BASE IS OPTIONAL, PLEASE SPECIFY IF BASE WILL BE REQUIRED.
- 7). WIRE IN ACCORDANCE WITH NATIONAL ELECTRICAL CODE USING COPPER TYPE WIRING.
- 8). CUSTOMER TO FURNISH MOUNTING HARDWARE.

VIEW: A

VIEW: B

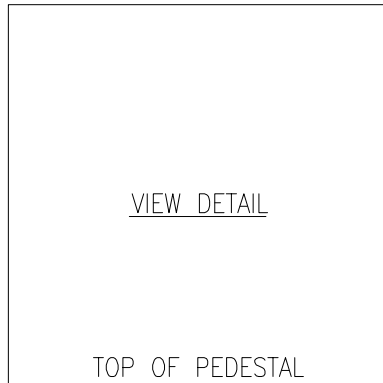

VIEW: C

PARTS LIST	
ITEM	DESCRIPTION
HOSPITAL GRADE RECEPTACLES	
1	DUPLEX RECEPTACLE - 20AMP/125V, IVORY
2	DUPLEX RECEPTACLE - 20AMP/125V, RED
3	SIMPLEX RECEPTACLE - 20AMP/125V, IVORY
4	SIMPLEX RECEPTACLE - 20AMP/125V, RED
TWIST-LOCK DEVICES	
5	TWIST-LOCK RECEPTACLE- SPECIFY NEMA CONFIGURATION NEMA:
6	GROUND JACK RECEPTACLE - 30AMP
MEDICAL GAS OUTLETS - CONSOLE TYPE ONLY	
<input type="checkbox"/> PROVISION ONLY <input type="checkbox"/> SUPPLIED BY POST GLOVER	
MFG.:	STYLE:
7	MEDICAL AIR
8	OXYGEN
9	VACUUM
MEDICAL GAS ACCESSORIES	
10	BOTTLE SLIDE BRACKET

ECN#04-239. UPDATED PER COMMENTS.

JJM | 10/15/04 | 01

REVISIONS

FOR:

FOR REFERENCE ONLY

S.O. NUM.:

STD. ORPD04008.xls ACAD STD.: ORPD04008.dwg
 B.O.M.:

TITLE/DESCRIPTION:
 OPERATING ROOM PEDESTAL
 PARTS LIST KEY AND GENERAL NOTES
 PAGE 2 OF 2



POST GLOVER LIFELINK
 4750 OLYMPIC BLVD. BLDG. B
 ERLANGER, KY U.S.A. 41018 (859) 283-5900
 COPYRIGHT © 2004

THIS DOCUMENT AND THE INFORMATION IT CONTAINS ARE THE PROPERTY OF POST GLOVER LIFELINK. IT IS DISCLOSED FOR THE PURPOSE FOR WHICH IT IS FURNISHED AND SHALL NOT BE DUPLICATED OR DISTRIBUTED.

DFTR: JJM DATE: 09/03/04 DWG. NO.: **ORPD04008** REV.: **01**